S-Lock®
User Manual

Thompson Retractor

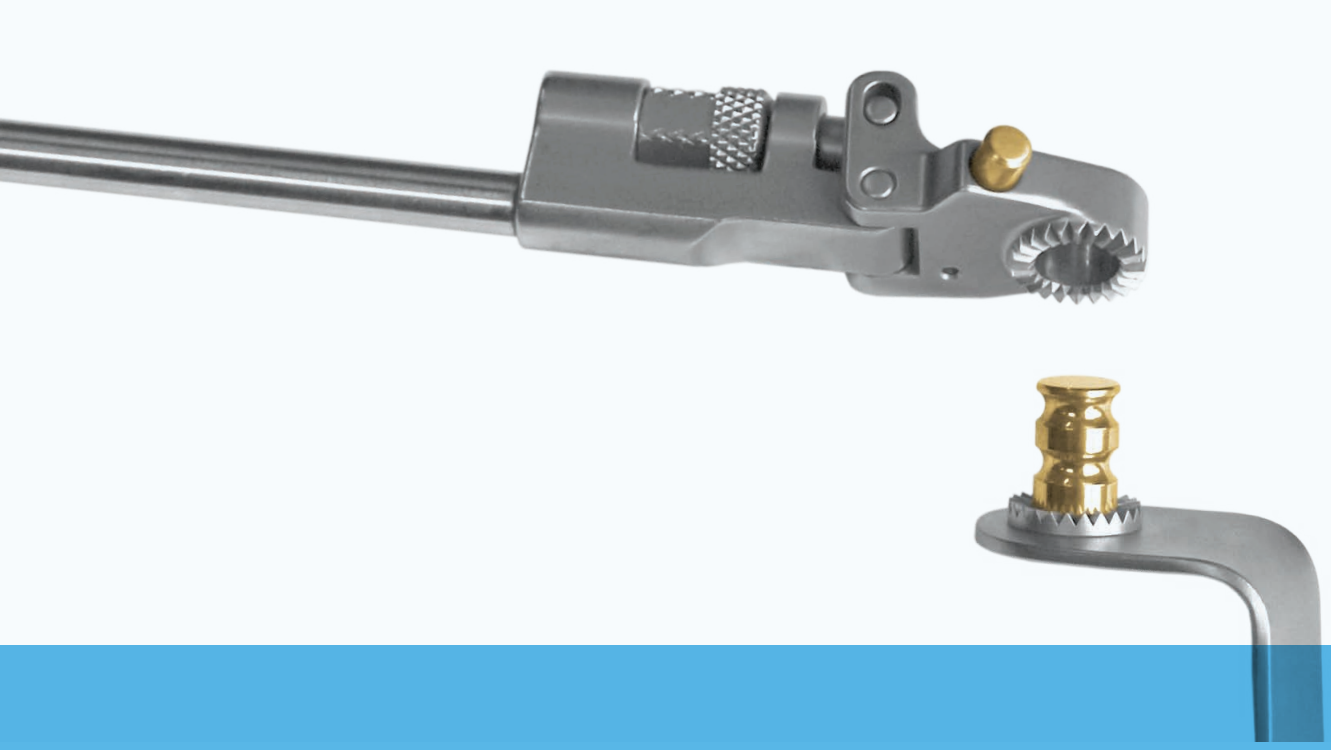

Uncompromised Exposure.

All S-Lock blade and handle part numbers start with an 'SL' or 'SO' and are only compatible with other S-Lock blades and handles.

1 COMBINE S-LOCK BLADE AND HANDLE

S-Lock handles have serrated faces that match up with serrations on S-Lock blades for precise blade placement.

Insert S-Lock blade nipple into S-Lock handle by pushing button.

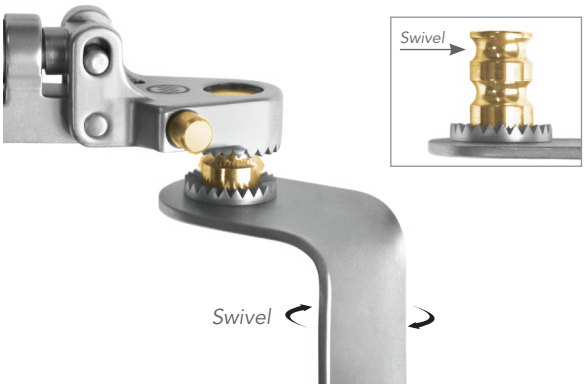

2 SWIVEL ALIGNS ON TISSUE

Release button with handle on the "swivel" groove nipple setting and swivel to desired position. Ensure the button is fully extended out of the handle to secure.

TIP: When in swivel position, nipple should be seated inside handle head, just below flush (as pictured).

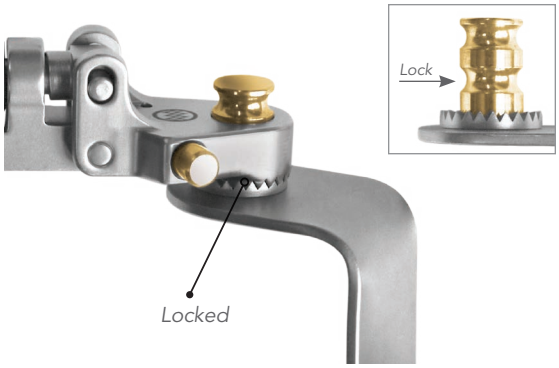

3 LOCK WHEN SWIVEL IS NOT DESIRED

Lock S-Lock blade in position on the "lock" groove nipple setting by pushing the button again and pressing straight down over the handle to engage the serrations. Ensure the button is fully extended out of the handle to secure.

TIP: To switch between two settings during use, unlock the handle or release retraction for ease of use.

4 RELEASING BLADES

Press button in to disengage.

NOTE: Blades with 'SO' before part number swivel only and do not lock in any orientation. 'SO' blades must only be used with 'SL' handles.

Thompson SURGICAL INSTRUMENTS

10170 East Cherry Bend Road
Traverse City, Michigan 49684
phone: 231.922.0177
fax: 231.922.0174

thompsonsurgical.com

Made in the USA

EC REP

Emergo Europe
Molenstraat 15
2513 BH, The Hague
THE NETHERLANDS

CE 0297

© 2014 Thompson Surgical Instruments, Inc. Traverse City, Michigan.
® S-Lock® and the T-Circle Logomark are Registered Trademarks of Thompson Surgical Instruments, Inc.
Patents: US4971038, US5025780, US5888197, US5897087, US5902233, US5984865, US6017008, US6033363, US6416465, US6511423, US7338442, US7749163, US8257255, US8360971, US8617064. Other patents pending.

Rev B
061714
dc slum0614